MIDMARK®

Installation Instructions

153657 Assistant's Instrument Tray

KIT COMPONENTS

Part Number	Description	Qty.
029-2732-00	Tray System, 12" (30.5 cm) x 14" (35.5 cm)	1
• 003-1240-00	Installation Instructions	1

REQUIRED TOOLS

Allen Wrenches (5 / 64", 1/8" and 5 / 32").
Level

INSTALLATION

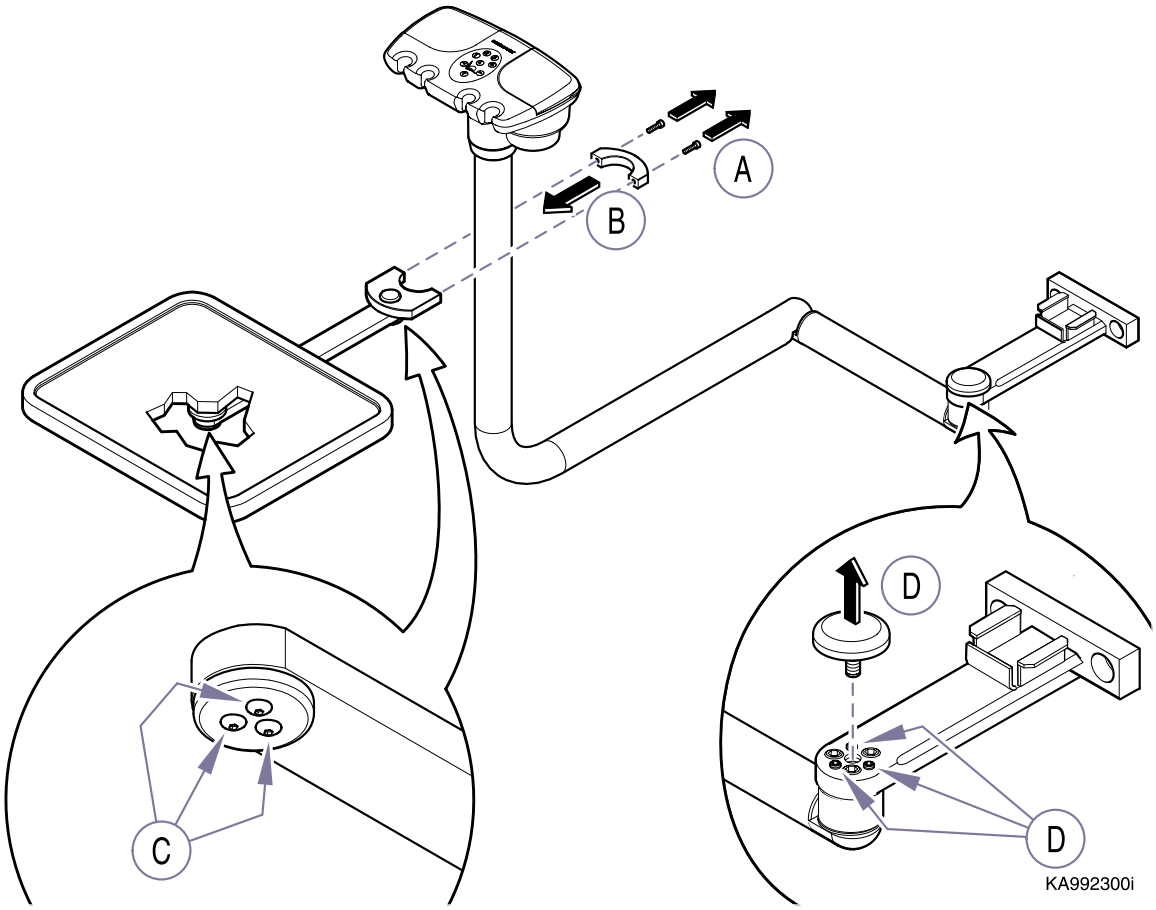

A. Remove the socket head screws and separate the two halves of the tray clamp.

B. Place the tray and clamp assembly in position on the assistant's instrument arm assembly and install the socket head screws.

C. Check operation. If necessary, the amount of drag at the two pivot points on the tray arm can be adjusted by tightening or loosening the three socket head screws at each location.

NOTE

Check the instrument arm to assure it is level. If necessary, adjust the three leveling screws.

D. Remove the cover and adjust the three leveling screws.

EQUIPMENT ALERT

Maximum shelf load limitation is 10 lbs. (4.5 kg).

© Midmark Corporation - 2001

MIDMARK®
Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542